



Appendix E

Noise Monitoring Equipment Calibration Certificate

Certificate of Calibration

for

Description: *Sound Level Calibrator*

Manufacturer: *RION*

Type No.: *NC-75*

Serial No.: *35124527*

Submitted by:

Customer: *Acuity Sustainability Consulting Limited*

Address: *Unit E, 12/F, Ford Glory Plaza,*

Nos. 37-39 Wing Hong Street,

Cheung Sha Wan, Kowloon,

Hong Kong

Upon receipt for calibration, the instrument was found to be:

☒ **Within**

☐ **Outside**

the allowable tolerance.

The test equipments used for calibration are traceable to National Standards via:

- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 19 October 2023

Date of calibration: 27 October 2023

Date of NEXT calibration: 26 October 2024

Calibrated by: 
Calibration Technician

Certified by: 
Mr. Ng Yan Wa
Laboratory Manager

Date of issue: 27 October 2023

Certificate No.: APJ23-090-CC002



Page 1 of 2

1. Calibration Precautions:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Specifications:

Calibration check

3. Calibration Conditions:

Air Temperature: 24.4 °C
Air Pressure: 1013 hPa
Relative Humidity: 65.4 %

4. Calibration Equipment:

| Test Equipment | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|------------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV220061 | HOKLAS |
| Sound Level Meter | RION NA-28 | 30721812 | AV220120 | HOKLAS |

5. Calibration Results**5.1 Sound Pressure Level**

| Nominal value dB | Accept lower level dB | Accept upper level dB | Measured value dB |
|---------------------|--------------------------|--------------------------|----------------------|
| 94.0 | 93.6 | 94.4 | 94.0 |

Note:

The values given in this certification only related to the values measured at the time of the calibration.

Certificate of Calibration

for

Description: *Sound Level Meter*
Manufacturer: *SVANTEK*
Type No.: *Svan 971 (Serial No.: 77731)*
Microphone: *BA3871 (Serial No.: 13905)*
Preamplifier: *SV18 (Serial No.: 121481)*

Submitted by:

Customer: *Acuity Sustainability Consulting Limited*
Address: *Unit E, 12/F, Ford Glory Plaza,
Nos. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon, Hong Kong*

Upon receipt for calibration, the instrument was found to be:

- ☒ **Within (31.5Hz – 8kHz)**
☐ **Outside**

the allowable tolerance.

The test equipment used for calibration are traceable to National Standards via:

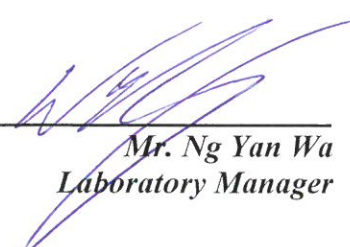
- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 16 March 2023

Date of calibration: 21 March 2023

Date of NEXT calibration: 20 March 2024

Calibrated by: 
Calibration Technician

Certified by: 
Mr. Ng Yan Wa
Laboratory Manager

Date of issue: 21 March 2023

Certificate No.: APJ22-157-CC001



Page 1 of 4

1. Calibration Precaution:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Conditions:

Air Temperature: 22.1 °C
Air Pressure: 1003 hPa
Relative Humidity: 62.2 %

3. Calibration Equipment:

| | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|----------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV220061 | HOKLAS |

4. Calibration Results

Sound Pressure Level

Reference Sound Pressure Level

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|--|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | | Level, dB | Frequency, Hz | dB | Specification, dB |
| 20-120 | dBA SPL | Fast | | 94 | 1000 | 94.1 | ±0.4 |

Linearity

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|--|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | | Level, dB | Frequency, Hz | dB | Specification, dB |
| 20-120 | dBA SPL | Fast | | 94 | 1000 | 94.1 | Ref |
| | | | | 104 | | 104.1 | ±0.3 |
| | | | | 114 | | 114.1 | ±0.3 |

Time Weighting

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|--|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | | Level, dB | Frequency, Hz | dB | Specification, dB |
| 20-120 | dBA SPL | Fast | | 94 | 1000 | 94.1 | Ref |
| | | Slow | | | | 94.1 | ±0.3 |

Certificate No.: APJ22-157-CC001



Page 2 of 4

Frequency Response

Linear Response

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 20-120 | dB | SPL | 94 | 31.5 | 94.2 | ±2.0 |
| | | | | 63 | 94.2 | ±1.5 |
| | | | | 125 | 94.2 | ±1.5 |
| | | | | 250 | 94.1 | ±1.4 |
| | | | | 500 | 94.1 | ±1.4 |
| | | | | 1000 | 94.1 | Ref |
| | | | | 2000 | 93.8 | ±1.6 |
| | | | | 4000 | 92.9 | ±1.6 |
| | | | | 8000 | 91.4 | +2.1; -3.1 |

A-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 20-120 | dBA | SPL | 94 | 31.5 | 54.9 | -39.4 ±2.0 |
| | | | | 63 | 68.1 | -26.2 ±1.5 |
| | | | | 125 | 78.1 | -16.1 ±1.5 |
| | | | | 250 | 85.5 | -8.6 ±1.4 |
| | | | | 500 | 90.9 | -3.2 ±1.4 |
| | | | | 1000 | 94.1 | Ref |
| | | | | 2000 | 95.0 | +1.2 ±1.6 |
| | | | | 4000 | 93.9 | +1.0 ±1.6 |
| | | | | 8000 | 90.5 | -1.1 ±2.1; -3.1 |

C-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 20-120 | dBC | SPL | 94 | 31.5 | 91.2 | -3.0 ±2.0 |
| | | | | 63 | 93.4 | -0.8 ±1.5 |
| | | | | 125 | 94.0 | -0.2 ±1.5 |
| | | | | 250 | 94.1 | -0.0 ±1.4 |
| | | | | 500 | 94.2 | -0.0 ±1.4 |
| | | | | 1000 | 94.1 | Ref |
| | | | | 2000 | 93.6 | -0.2 ±1.6 |
| | | | | 4000 | 92.1 | -0.8 ±1.6 |
| | | | | 8000 | 88.6 | -3.0 +2.1; -3.1 |

Certificate No.: APJ22-157-CC001



Page 3 of 4



5. Calibration Results Applied

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:

| | | |
|--------|---------|--------|
| 94 dB | 31.5 Hz | ± 0.15 |
| | 63 Hz | ± 0.10 |
| | 125 Hz | ± 0.05 |
| | 250 Hz | ± 0.10 |
| | 500 Hz | ± 0.10 |
| | 1000 Hz | ± 0.05 |
| | 2000 Hz | ± 0.05 |
| | 4000 Hz | ± 0.05 |
| | 8000 Hz | ± 0.10 |
| 104 dB | 1000 Hz | ± 0.05 |
| 114 dB | 1000 Hz | ± 0.05 |

The uncertainties are evaluated for a 95% confidence level.

Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)*L shall not be liable for any loss or damage resulting from the use of the equipment.

Certificate No.: APJ22-157-CC001



Page 4 of 4

Certificate of Calibration

for

Description: *Sound Level Meter*
Manufacturer: *SVANTEK*
Type No.: *SVAN 971 (Serial No.:C132261)*
Microphone: *SV 7052E (Serial No.: 79778)*
Preamplifier: *SVANTEK SV-18 (Serial No.:97276)*

Submitted by:

Customer: *Acuity Sustainability Consulting Limited*
Address: *Unit E, 12/F, Ford Glory Plaza,
Nos. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon, Hong Kong*

Upon receipt for calibration, the instrument was found to be:

- ☒ **Within (31.5Hz – 4kHz)**
☐ **Outside**

the allowable tolerance.

The test equipment used for calibration are traceable to National Standards via:

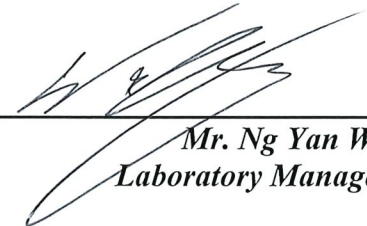
- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 19 October 2023

Date of calibration: 27 October 2023

Date of NEXT calibration: 26 October 2024

Calibrated by: 
Calibration Technician

Certified by: 
Mr. Ng Yan Wa
Laboratory Manager

Date of issue: 27 October 2023

Certificate No.: APJ23-091-CC006



Page 1 of 4

1. Calibration Precaution:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Conditions:

Air Temperature: 22.6 °C
Air Pressure: 1016 hPa
Relative Humidity: 65.3 %

3. Calibration Equipment:

| | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|----------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV220061 | HOKLAS |

4. Calibration Results

Sound Pressure Level

Reference Sound Pressure Level

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|---------------|---------------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | |
| 25-124.9 | dBA SPL | Fast | 94 | 1000 | 94.0 | ±0.4 |

Linearity

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|---------------|---------------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | |
| 25-124.9 | dBA SPL | Fast | 94 | 1000 | 94.0 | Ref |
| | | | 104 | | 104.0 | ±0.3 |
| | | | 114 | | 114.0 | ±0.3 |

Time Weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|---------------|---------------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | |
| 25-124.9 | dBA SPL | Fast | 94 | 1000 | 94.0 | Ref |
| | | Slow | | | 94.0 | ±0.3 |

Certificate No.: APJ23-091-CC006



Page 2 of 4

Frequency Response

Linear Response

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|---------------|---------------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | |
| 25-124.9 | dB | SPL | 94 | 31.5 | 94.4 | ±2.0 |
| | | | | 63 | 94.3 | ±1.5 |
| | | | | 125 | 94.2 | ±1.5 |
| | | | | 250 | 94.1 | ±1.4 |
| | | | | 500 | 94.1 | ±1.4 |
| | | | | 1000 | 94.0 | Ref |
| | | | | 2000 | 93.8 | ±1.6 |
| | | | | 4000 | 93.3 | ±1.6 |

A-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|---------------|---------------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | |
| 25-124.9 | dBA | SPL | 94 | 31.5 | 55.1 | -39.4 ±2.0 |
| | | | | 63 | 68.1 | -26.2 ±1.5 |
| | | | | 125 | 78.1 | -16.1 ±1.5 |
| | | | | 250 | 85.5 | -8.6 ±1.4 |
| | | | | 500 | 90.8 | -3.2 ±1.4 |
| | | | | 1000 | 94.0 | Ref |
| | | | | 2000 | 95.0 | +1.2 ±1.6 |
| | | | | 4000 | 94.3 | +1.0 ±1.6 |

C-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|---------------|---------------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | |
| 25-124.9 | dBC | SPL | 94 | 31.5 | 91.4 | -3.0 ±2.0 |
| | | | | 63 | 93.4 | -0.8 ±1.5 |
| | | | | 125 | 94.0 | -0.2 ±1.5 |
| | | | | 250 | 94.1 | -0.0 ±1.4 |
| | | | | 500 | 94.1 | -0.0 ±1.4 |
| | | | | 1000 | 94.0 | Ref |
| | | | | 2000 | 93.6 | -0.2 ±1.6 |
| | | | | 4000 | 92.5 | -0.8 ±1.6 |



5. *Calibration Results Applied*

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:

| | | |
|--------|---------|--------|
| 94 dB | 31.5 Hz | ± 0.10 |
| | 63 Hz | ± 0.10 |
| | 125 Hz | ± 0.05 |
| | 250 Hz | ± 0.05 |
| | 500 Hz | ± 0.05 |
| | 1000 Hz | ± 0.05 |
| | 2000 Hz | ± 0.05 |
| | 4000 Hz | ± 0.05 |
| 104 dB | 1000 Hz | ± 0.05 |
| 114 dB | 1000 Hz | ± 0.05 |

The uncertainties are evaluated for a 95% confidence level.

Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)*L shall not be liable for any loss or damage resulting from the use of the equipment.

Certificate No.: APJ23-091-CC006



Page 4 of 4